




Product Specification
**Serological pipette, plugged, 10 ml, sterile,
non-pyrogenic/endotoxin-free, non-cytotoxic, 1
piece(s)/blister**

Page 1

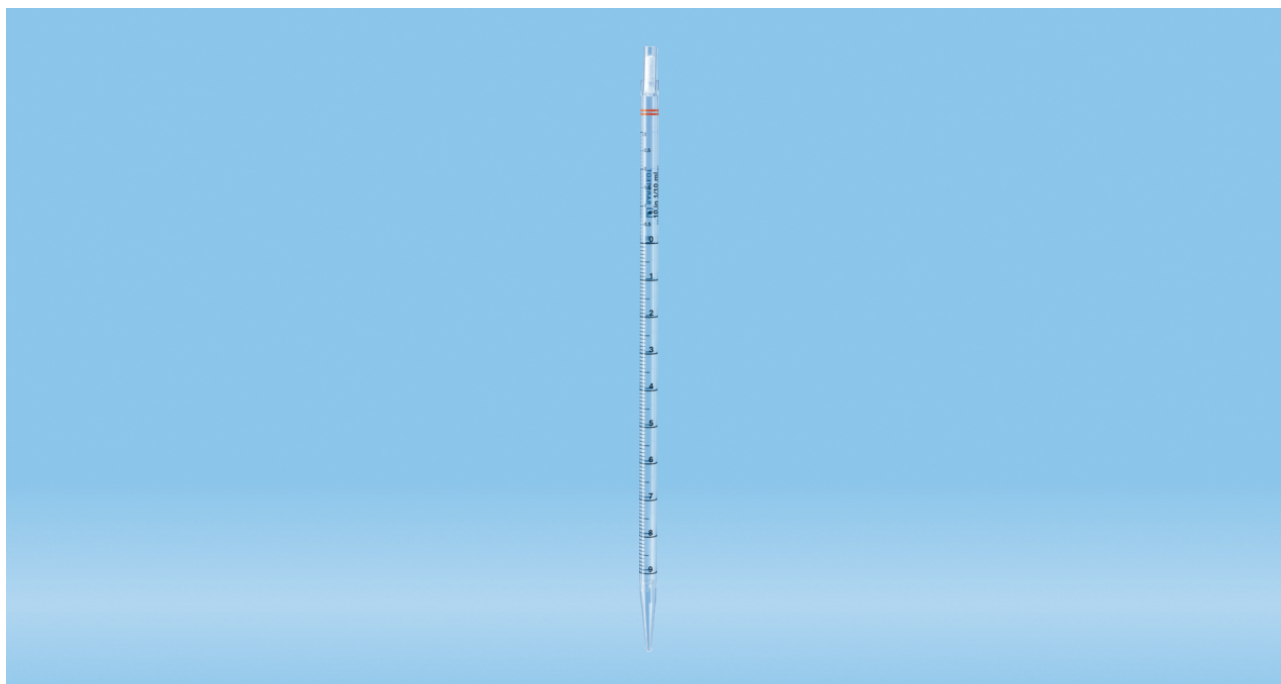

Product description

Order number	86.1254.001
Product description	Serological pipette, plugged, max. working volume: 10 ml, coding colour: orange, material: PS, sterile, non-pyrogenic/endotoxin-free, non-cytotoxic, 1 piece(s)/blister

Product characteristics

Colour of print/label	orange
Graduation	yes
Design	plugged
Volume of work	10 ml
Coding colour	orange

This is the current specification for this product. Sarstedt reserves the right to make changes, in full or in part, at any time without prior notification.

This specification is confidential and the property of Sarstedt. It is neither to be duplicated nor made available to third parties without our prior written consent.

Date of issue:
2021-10-22

This document was prepared by EDP support and is valid without signature.



SARSTEDT



Product Specification
**Serological pipette, plugged, 10 ml, sterile,
non-pyrogenic/endotoxin-free, non-cytotoxic, 1
piece(s)/blister**

Page 2

Size

Diameter 10 mm
Length of product 335 mm

Material & colours

Product material Polystyrene (PS)
Colour of product transparent

Purity & certification

Product category no medical device | IVD
Purity standard sterile, non-pyrogenic/endotoxin-free, non-cytotoxic
Sterilisation Gamma irradiation
Pyrogen-free yes
Batched yes

Packaging

Minimum order qty. 500
Type of inner packaging blister
Piece(s) / inner box 50
Piece(s) / case 500
Piece(s) / pallet 27000
Case volume 0,0305 cbm
Weight of product 0,0104 kg
Weight of case 5,74 kg
EAN of inner box 4038917127295
EAN case 4038917021128

This is the current specification for this product. Sarstedt reserves the right to make changes, in full or in part, at any time without prior notification.

This specification is confidential and the property of Sarstedt. It is neither to be duplicated nor made available to third parties without our prior written consent.

Date of issue:
2021-10-22

This document was prepared by EDP support and is valid without signature.



SARSTEDT