




**Product Specification**  
**Serological pipette, plugged, 10 ml, sterile,  
non-pyrogenic/endotoxin-free, non-cytotoxic, 1  
piece(s)/blister**

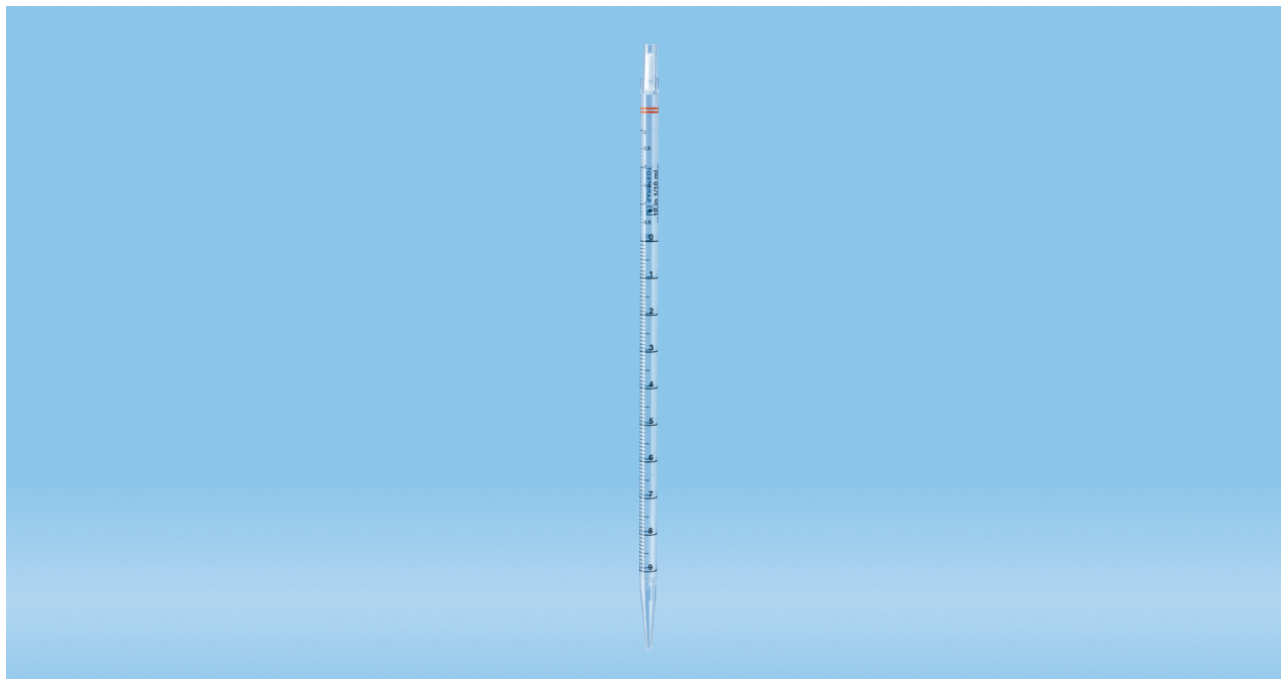

**Product description**

Order number	86.1254.001
Product description	Serological pipette, plugged, 10 ml, coding colour: orange, material: PS, sterile, non-pyrogenic/endotoxin-free, non-cytotoxic, 1 piece(s)/blister

**Product characteristics**

Colour of print/label	orange
Graduation	yes
Design	plugged
Volume of work	10 ml
Coding colour	orange

**Size**

Diameter	10 mm
Length of product	335 mm

This is the current specification for this product. Sarstedt reserves the right to make changes, in full or in part, at any time without prior notification.

This specification is confidential and the property of Sarstedt. It is neither to be duplicated nor made available to third parties without our prior written consent.





**Product Specification**  
**Serological pipette, plugged, 10 ml, sterile,  
non-pyrogenic/endotoxin-free, non-cytotoxic, 1  
piece(s)/blister**

**Page 2**

**Material & colours**

Product material Polystyrene (PS)  
Colour of product transparent

**Purity & certification**

Product category no medical device | IVD  
Purity standard sterile, non-pyrogenic/endotoxin-free, non-cytotoxic  
Sterilisation Gamma irradiation  
Pyrogen-free yes  
Batched yes

**Packaging**

Minimum order qty. 500  
Type of smallest blister  
subpackaging  
Piece(s) / inner box 50  
Piece (s) / outer case 500  
Piece(s) / pallet 27000  
Depth of case 420 mm  
Width of case 250 mm  
Height of case 290 mm  
Case volume 0.0305 cbm  
Weight of product 0.0104 kg  
Weight of case 5.74 kg  
EAN of inner box 4038917127295  
EAN case 4038917021128

This is the current specification for this product. Sarstedt reserves the right to make changes, in full or in part, at any time without prior notification.

This specification is confidential and the property of Sarstedt. It is neither to be duplicated nor made available to third parties without our prior written consent.

Date of issue:  
2023-01-27

This document was prepared by EDP support and is valid without signature.



**SARSTEDT**